


Condensation Particle Counter for Detecting Particles as Small as 1.5nm

Peter McMurry (PI), Kenjire Iida

Mechanical Engineering, University of Minnesota

NNIN Facility utilized: Particle Technology Lab

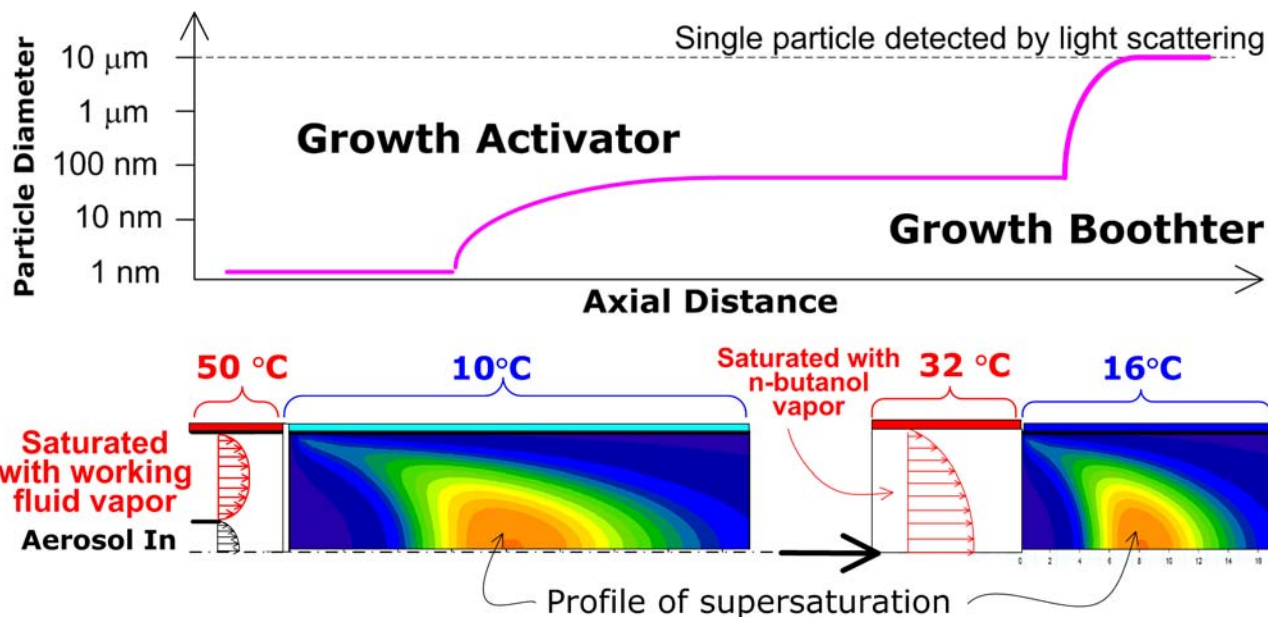

Experimental Results

- ❖ Diethylene glycol as working fluid
- ❖ NaCl as test particles
- ❖ Particle as small as 1nm could be detected

